

Pulse Oximetry Test: Summary Report - ID# 001067100

Patient Information

Tag tester Tester4

Insurance: Aetna

DOB : 6/2/1992

Gender : Male

Referring/Ordering Physician

Tagvignesh Pandian

NPI # : 9602230

Phone : (544) 212-1211

Fax : (999) 999-9999

DME/HME Courier (Respiratory Supplier)

HME Demo Account

6125 Sherwin Drive

Phone : (352) 293-2810

Fax : (727) 264-2117

Study Date : 12/14/2016

Device Type: CMS50F

RX Date : 1/10/2017 4:57:41 AM

Start Time : 12/14/2016 12:36:20 PM

Test Duration: 01:06:38

Oximeter SN : -

End Time : 12/14/2016 02:20:11 PM

Valid Time : 00:53:06

Test Condition : BIPAP™ w/ 9.5 LPM

SpO2 / Pulse Information

Highest SpO2 : 100%

SpO2 ≤ 88% : 00:28:19

Highest Pulse : 100 BPM

Awake SpO2 :99% (1st 5 Mins of Test)

Average SPO2 : 87 %

SpO2 ≤ 89% :00:31:36

Average Pulse : 97 BPM

Events Per Hour (ODI) : 0


Lowest SpO2 : 70%

Lowest Pulse : 86 BPM

Excluded Artifacts : 3

Qualification Status: Group 1 Qualifier Patient demonstrates saturation levels at or below 88% for five minutes or greater, taken during sleep, or a decrease in arterial oxygen saturation greater than 5% for at least five minutes, taken during sleep, with associated symptoms. Contact your local Medicare Contractor for more specifics on these diagnosis codes that support medical necessity.

SpO2 / Pulse Graphs

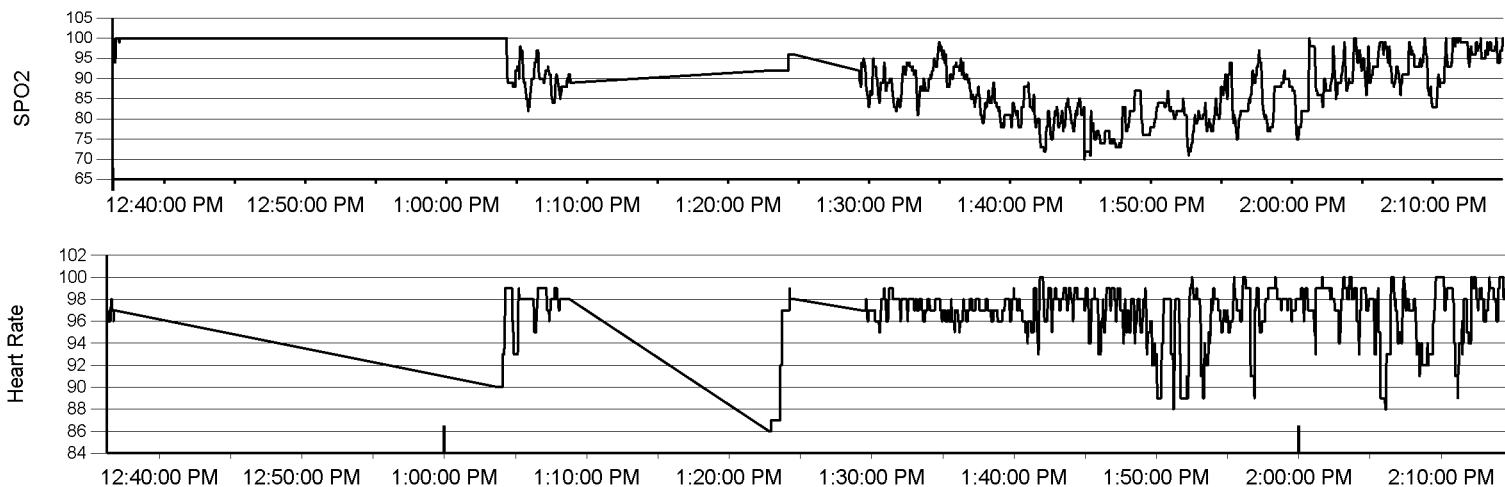

Oxygen Prescription

Tag tester Tester4 was seen on ___/___/___ for which I ordered an overnight oximetry test. These results, listed above, show that the patient's SpO2 drops throughout the night & would benefit from home oxygen. I Tagvignesh Pandian, am ordering nocturnal oxygen at ___ LPM, via nasal cannula, today as part of Tag tester Tester4 's plan of care. Once signed, please fax this form to HME Demo Account at (727) 264-2117.

Physician Signature: _____

Order/Signature Date: ___/___/___



Physician: Tagvignesh Pandian | NPI: 9602230

This oximeter was uploaded by HME Demo Account on 1/11/2017 5:06:30 AM.
HDMS Account#:

Patient: Tag tester Tester4
DOB: 6/2/1992
Test Start Time: 12/14/2016 12:36:20 PM

Ordering Physician: Tagvignesh Pandian
Insurance: Aetna
Test End Time: 12/14/2016 2:20:11 PM

Pulse Oximetry Test: SpO₂ & Heart Graphs

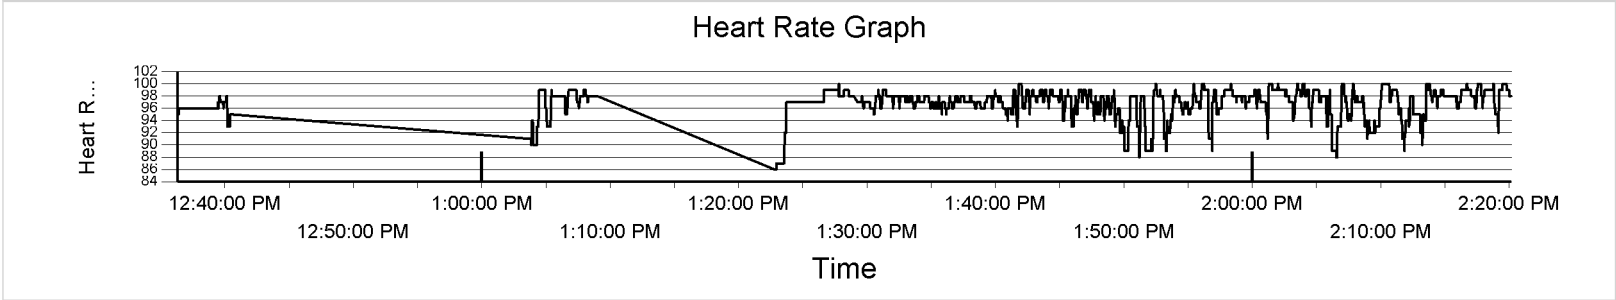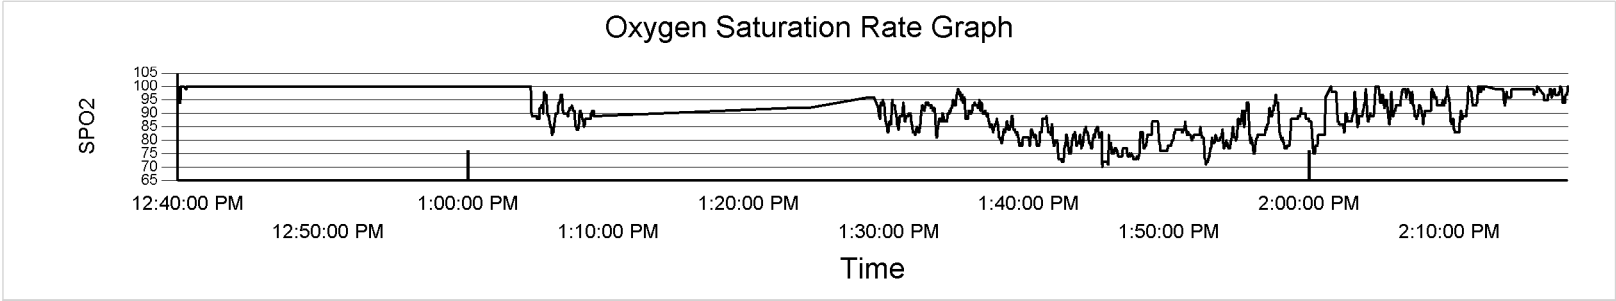



Patient: Tag tester Tester4
 DOB: 6/2/1992
 Test Start Time: 12/14/2016 12:36:20 PM

Ordering Physician: Tagvignesh Pandian
 Insurance: Aetna
 Test End Time: 12/14/2016 2:20:11 PM

Pulse Oximetry Test: SpO₂ & Pulse Breakdown

Percentage of Time Spent Page : This page will show a breakdown of the Pulse Oximetry Test at the individual SpO₂ percentages from 99% - 40%.

SPO2 : 90	3.93 % time	SPO2 : 80	2.55 % time	SPO2 : 70	0.03 % time
SPO2 : 91	3.43 % time	SPO2 : 81	2.85 % time	SPO2 : 71	0.15 % time
SPO2 : 92	4.16 % time	SPO2 : 82	5.01 % time	SPO2 : 72	0.98 % time
SPO2 : 93	4.71 % time	SPO2 : 83	3.73 % time	SPO2 : 73	0.93 % time
SPO2 : 94	2.85 % time	SPO2 : 84	3.1 % time	SPO2 : 74	1.13 % time
SPO2 : 95	1.68 % time	SPO2 : 85	2.18 % time	SPO2 : 75	1.4 % time
SPO2 : 96	2.5 % time	SPO2 : 86	2.58 % time	SPO2 : 76	1.23 % time
SPO2 : 97	2.35 % time	SPO2 : 87	3.53 % time	SPO2 : 77	1.9 % time
SPO2 : 98	2.25 % time	SPO2 : 88	4.21 % time	SPO2 : 78	2.93 % time
SPO2 : 99	2.35 % time	SPO2 : 89	4.93 % time	SPO2 : 79	2.13 % time
Total 90'S	30.21 % time	Total 80'S	34.67 % time	Total 70'S	12.81 % time
SPO2 : 60	0.0 % time	SPO2 : 50	0.0 % time	SPO2 : 40	0.0 % time
SPO2 : 61	0.0 % time	SPO2 : 51	0.0 % time	SPO2 : 41	0.0 % time
SPO2 : 62	0.0 % time	SPO2 : 52	0.0 % time	SPO2 : 42	0.0 % time
SPO2 : 63	0.0 % time	SPO2 : 53	0.0 % time	SPO2 : 43	0.0 % time
SPO2 : 64	0.0 % time	SPO2 : 54	0.0 % time	SPO2 : 44	0.0 % time
SPO2 : 65	0.0 % time	SPO2 : 55	0.0 % time	SPO2 : 45	0.0 % time
SPO2 : 66	0.0 % time	SPO2 : 56	0.0 % time	SPO2 : 46	0.0 % time
SPO2 : 67	0.0 % time	SPO2 : 57	0.0 % time	SPO2 : 47	0.0 % time
SPO2 : 68	0.0 % time	SPO2 : 58	0.0 % time	SPO2 : 48	0.0 % time
SPO2 : 69	0.0 % time	SPO2 : 59	0.0 % time	SPO2 : 49	0.0 % time
Total 60'S	0 % time	Total 50'S	0 % time	Total 40'S	0 % time

SpO₂ Time Breakdown

SpO ₂ Time <90% :	00:31:36	SpO ₂ Time ≥ 90% :	00:21:27
SpO ₂ Time <80% :	00:08:31	SpO ₂ Time ≥ 80% & <90% :	00:23:05
SpO ₂ Time <70% :	00:00:00	SpO ₂ Time ≥ 70% & <80% :	00:08:31
SpO ₂ Time <60% :	00:00:00	SpO ₂ Time ≥ 60% & <70% :	00:00:00

Pulse Percentage Breakdown

Pulse Range > 199	0.00 %	Pulse Range 90 - 99	92.05 %
Pulse Range 180 - 199	0.00 %	Pulse Range 80 - 89	3.99 %
Pulse Range 160 - 179	0.00 %	Pulse Range 70 - 79	0.00 %
Pulse Range 140 - 159	0.00 %	Pulse Range 60 - 69	0.00 %
Pulse Range 120 - 139	0.00 %	Pulse Range 50 - 59	0.00 %
Pulse Range 100 - 119	3.96 %	Pulse Range < 50	0.00 %